




Printout Sample

- 1 Subjective refraction Far VA value
- 2 Subjective refraction Near VA value
- 3 Grid test result
- 4 Glare test result
- 5 Contrast test result
- 6 Far VA for lensmeter
- 7 Near VA for lensmeter
- 8 Glare test VA for lensmeter
- 9 Contrast test VA for lensmeter


OID : -KR 010001-	
NAME	
2013_12_24	AM 10:00
No. 0001	01
SN:	
SBJ. DATA(REF)	
(R) S C A VA	
-5.00 -2.00 75 0	
(L) S C A VA	
-0.25 -1.00 90 1.2	
NEAR TEST(REF)	
(R) DIST. ADD VA	
40 cm +2.50 0	
(L) DIST. ADD VA	
33 cm +2.25 1.2	
GRID CHART(REF)	
(R) (L)	
TS: NG NS: NG NS: OK TS: OK	
C: NG C: OK	
TI: OK NI: OK NI: OK TI: NG	
GLARE TEST(REF)	
(R) (L)	
VA 0.6 VA 0.6	
CONTRAST TEST(REF)	
(R) VA LVL (L) VA LVL	
0.8 50% 1.0 50%	
SBJ. DATA(CL)	
(R) S C A VA	
-2.00 -1.00 95 0.6	
(L) S C A VA	
-0.25 -1.00 100 1.2	
NEAR TEST(CL)	
(R) DIST. ADD VA	
40 cm +1.00 0.5	
(L) DIST. ADD VA	
33 cm +1.00 0.	
GLARE TEST(CL)	
(R) (L)	
VA 0.3 VA 0.6	
CONTRAST TEST(CL)	
(R) (L)	
VA 0.5 VA 0.7	
LVL 50% LVL 25%	
TOPCON	

Sample

Chart thumbnail

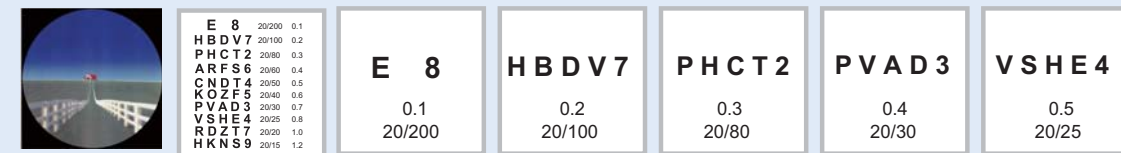

Objective chart Subjective chart

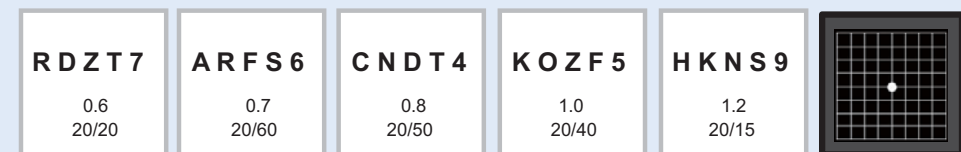


Grid chart

Specifications

Refractive Power Measurement	Spherical refractive power	-25D to +22D (0.12D/0.25D steps) ※
	Cylindrical refractive power	OD to $\pm 10D$ (0.12D/0.25D steps) ※
	Astigmatic axial angle	0° to 180° (in 1° or 5° steps)
	Minimal measurable pupil diameter	$\phi 2$ mm
Corneal Curvature Measurement	Corneal curvature radius	5.00 to 10.00mm (0.01mm step)
	Corneal refractive power	67.50D to 33.75D (0.12D/0.25D steps) (where, corneal refractive power = 1.3375)
	Corneal astigmatic refractive power	OD to $\pm 10D$ (0.12D/0.25 D steps)
	Corneal astigmatic axial angle	0° to 180° (1°/ 5° steps)
Range of Subjective refractive check	pherical refractive power:	Spherical refractive power: -18D to +18D (0.25D steps)
	Test chart:	Eyesight test chart of 0.1 to 1.2 or 20/200 to 20/15, Grid display
	Chart display:	Overall, Horizontal series, Contrast change
	Test items:	Far-sightedness, Near-sightedness, Glare test
PD Measurement Range		20mm to 85mm (0.5mm step)
Data Transport Terminal		USB (Import) /RS-232C (Import/Export) / LAN (Export)
Dimensions		317-341mm (W) × 521-538mm (D) × 447-477 mm (H)
Weight		15 kg
Power Supply		100-240V AC, 50-60Hz, 70VA

※ -25D \cong spherical refractive power + cylindrical refractive power or spherical refractive power + cylindrical refractive power \cong +22D

System chart

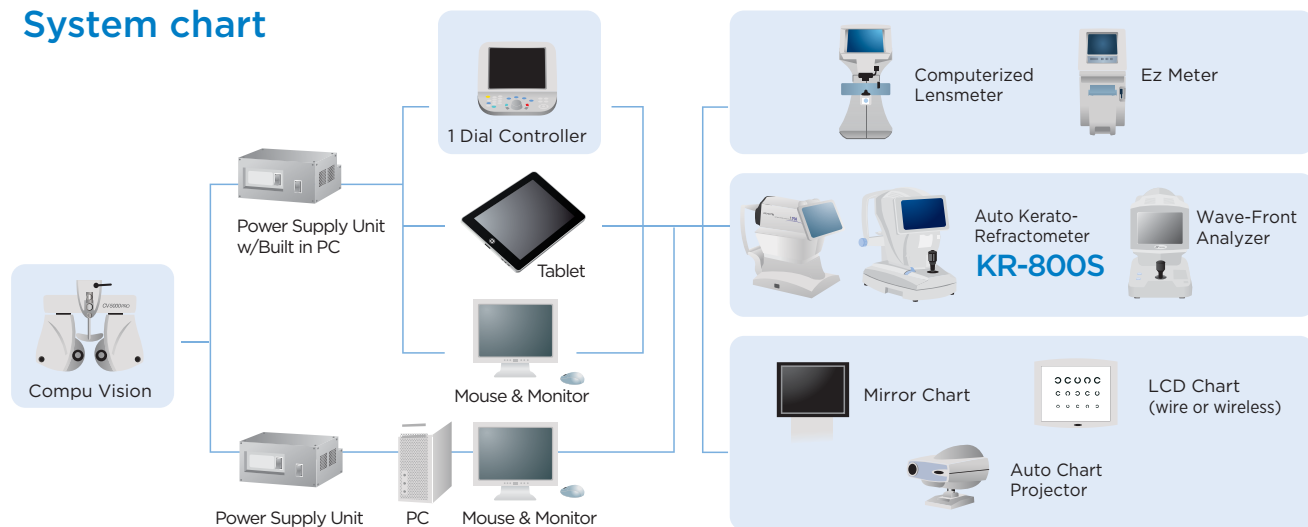

* Please contact Topcon subsidiaries or dealers for system configurations.



* Not available in all countries, please check with your distributor for availability in your country
 * Subject to change in design and/or specifications without advanced notice.

IMPORTANT

In order to obtain the best results with this instrument,
 please be sure to review all user instructions prior to operation.



TOPCON CORPORATION

75-1 Hasunuma-cho, Itabashi-ku, Tokyo 174-8580, Japan. Phone: +81-(0)3-3558-2522/2502 Fax: +81-(0)3-3965-6898 www.topcon.co.jp

TOPCON MEDICAL SYSTEMS, INC.
 111 Baxter Drive, Oakland, NJ 07438, U.S.A.
 Phone: +1-201-589-3300 Fax: +1-201-589-5250 www.topconmedical.com

TOPCON CANADA INC.
 110 Provencher Avenue, Boisbriand, QC J7G 1N1 CANADA
 Phone: +1-514-450-7771 Fax: +1-514-450-6467 www.topcon.ca

TOPCON EUROPE MEDICAL B.V.
 Esseebaan 11, 2908 LJ Capelle a/d IJssel, P.O. Box 145,
 2900 AC Capelle a/d IJssel, THE NETHERLANDS
 Phone: +31-(0)10-455077 Fax: +31-(0)10-455045
 E-mail: medical@topcon.eu www.topcon-medical.eu

ITALY OFFICE
 Viale dell'Industria 60, 20037 Paderno Dugnano, (Milano), ITALY
 Phone: +39-02-986671 Fax: +39-02-9808091 E-mail: info@topcon.it www.topcon.it

DANMARK OFFICE
 Præstemarkvej 25, 4000 Roskilde, DANMARK
 Phone: +45-46-327500 Fax: +45-46-327555
 E-mail: topcon@topcondanmark.dk www.topcondanmark.dk

IRELAND OFFICE
 Unit 276, Blanchardstown, Corporate Park 2 Ballycoolin Dublin 15, IRELAND
 Phone: +353-8975900 Fax: +353-8293915 E-mail: medical@topcon.ie www.topcon.ie

TOPCON S.A.R.L.
 BAI Al 3 route de la rovette 93205 SAINT DENIS CEDEX
 Phone: +33-1-49-21-23-23 Fax: +33-1-49-21-23-24 E-mail: topcon@topcon.fr www.topcon.fr

TOPCON DEUTSCHLAND MEDICAL G.m.b.H.
 Hems-Martin-Schäfer Strasse 41 D-47877 Willich, GERMANY
 Phone: +49-(0)2054-8850 Fax: +49-(0)2054-88517 E-mail: med@topcon.de www.topcon.de

TOPCON SCANDINAVIA A.B.
 Neogatan 2, P.O. Box 25, 43151 Mölndal, SWEDEN
 Phone: +46-(0)31-7109200 Fax: +46-(0)31-7109249 E-mail: medical@topcon.se www.topcon.se

TOPCON ESPAÑA S.A.
 Head Office
 Frederic Montpou 4 Etc. A Bajas 3, 08960 Sant Just Desvern Barcelona, SPAIN
 Phone: +34-93-4754057 Fax: +34-93-4733932 E-mail: medical@topcon.es www.topcon.es

TOPCON (GREAT BRITAIN) LTD.
 Topcon House, Kismet Side Lane, Newbury, Berkshire RG14 5PX United Kingdom
 Phone: +44-(0)1635-551120 Fax: +44-(0)1635-551170 E-mail: medical@topcon.co.uk www.topcon.co.uk

TOPCON POLSKA Sp. z o.o.
 ul. Warszawska 23, 42-470 Siewierz, POLAND
 Phone: +48-(0)32-6705945 Fax: +48-(0)32-6713405 www.topcon-polska.pl



TOPCON CORPORATION



TOPCON CORPORATION



TOPCON CORPORATION

TOPCON SINGAPORE MEDICAL PTE. LTD.
 JALAN KILANG TIMOR #09-01 PACIFIC TECH CENTRE SINGAPORE 159303
 Phone: +65-68120606 Fax: +65-6775650
 E-mail: medical_sales@topcon.sg www.topcon.com.sg

REPRESENTATIVE OFFICE IN INDONESIA
 Level 38, Tower A, Kota Kasablanka unit G4-04, Jl.
 Casablanca, Kav 88, Jakarta, Indonesia 12870
 Phone: +62-21-2963-8004

TOPCON INSTRUMENTS (MALAYSIA) SDN.BHD.
 No. 01, (Ground Floor), Jalan Excelia 2, Off Jalan Ampang Putra,
 Taman Ampang Hilir, 55100 Kuala Lumpur, MALAYSIA
 Phone: +60-(0)3-42709866 Fax: +60-(0)3-42709786

TOPCON INSTRUMENTS (THAILAND) CO., LTD.
 77/62 Srinisathorn Tower, 37th Floor, Khungthorburd Rd, Klongtoisai,
 Klongsarn, Bangkok 10600, THAILAND
 Phone: +66-(0)2-440-1152-7 Fax: +66-(0)2-440-1158

KR-800S

Auto Kerato-Refractometer



PERFORMANCE
 YOU CAN COUNT ON



More Than Just an Auto Kerato Refractometer

The sleek and modern design of the KR-800S incorporates the latest technology designed to increase practice efficiency and enhance the patient experience. The KR-800S provides auto refraction, keratometry, contrast screening, visual acuity, and glare testing all in one easy to use instrument.

This multi-functionality supports enhanced work flow, and enables the KR-800S to be used in any variety of settings from hospitals, multi-specialty ophthalmic and optometric clinics and even vision screening centers.

- » Enhances workflow efficiency and improves utilization.
- » Comfortable and smooth examination provides superior patient experience
- » Assessment of visual acuity under glare conditions
- » Multi-functional instrument helps you quickly document the patient's vision during treatment and follow up of a range of ocular diseases
- » Small footprint and LAN connection supports flexible installation.



KR-800S

Auto Kerato-Refractometer

KR-800S will dramatically change
the clinical workflow

Subjective
VA Test

Subjective
IOL Type
Selection

Grid Test

Glare Test

Contrast
Test

Objective
Test




Range of functions

Objective and Subjective Data



KR-800S displays the test results of all objective and subjective measurements on a single screen. This all-in-one instrument saves examination time and offers wide functionality in situations where a manual refractor is not available, such as school screening, athletic or occupational screening, and nursing homes. Refractive results can be viewed on the screen, printed out, or exported to an Electronic Health Record.


Objective Test

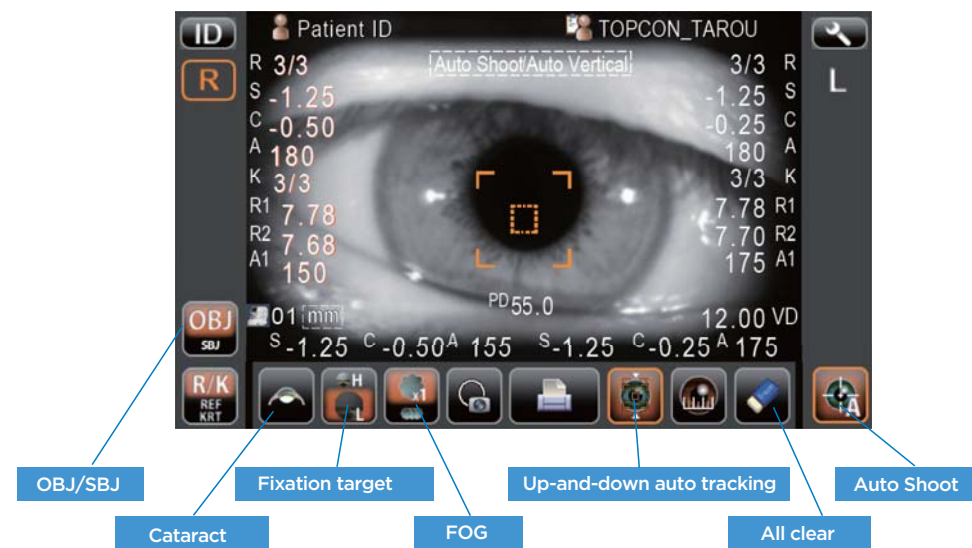

Subjective Test

All information is shown on the one screen

Lensmeter results, Objective results, Subjective results, and Spherical Equivalent simulation are displayed. The operator can refer to all of the information during the subjective tests.

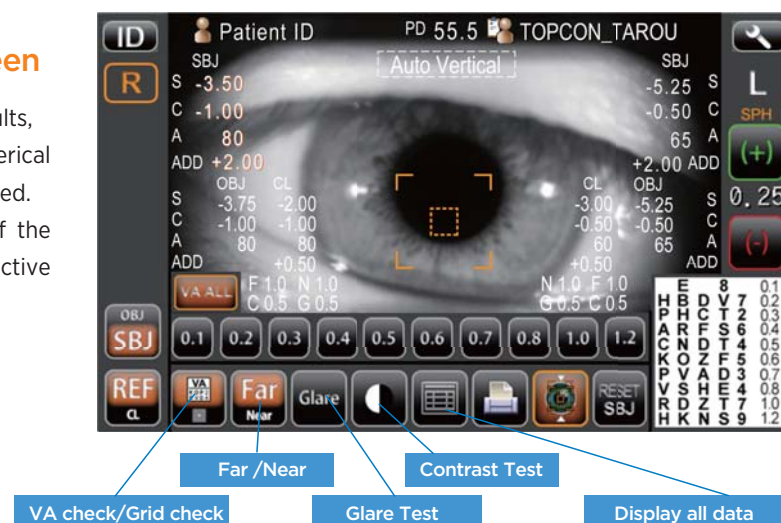

Glare test



The test is simple, standardized and provides a consistent and reliable way to evaluate vision changes in the presence of bright lights.

*The Glare test can only be performed with the subjective far distance test.



Glare Vision



Example

Normal Vision




Example

Contrast test



The contrast test is an ideal test to check the patient's quality of vision. The contrast of the chart can be changed across a range of percentages.


* The Contrast test can only be performed with the subjective far distance test.
* Only the contrast of the background changes.

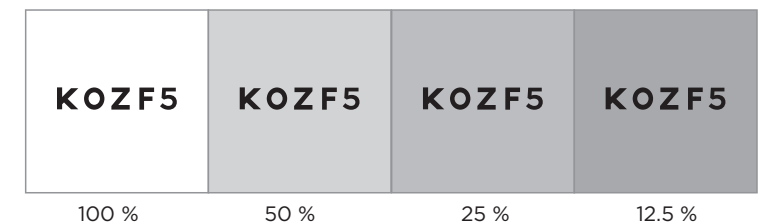

Grid test




The grid test can be performed for conditions affecting the macula. Patients with macular disease may see wavy or missing lines. The test can be helpful in detecting early signs of abnormality in the eye. New grid test function shows the grid for no longer than 0.25 seconds to prevent the natural "completion phenomenon" filling in the grid.

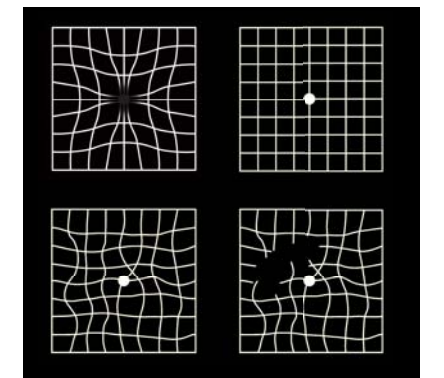

What is Completion phenomenon?

The human brain is able to restore "crooked" lines back to straight lines in just over 0.25 seconds, losing the actual result

*The Grid test can only be performed with the subjective far distance test.

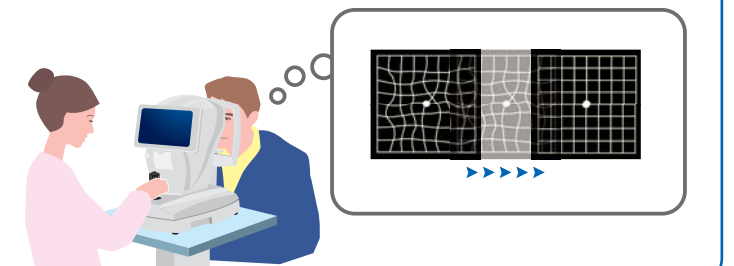

Other Features

Compare toric to non toric correction




This software function allows the patient to visualize the potential post-surgical difference between a spherical and toric IOL. Simply push a single button to switch “Sphere, Cylinder, and Axis” to “Spherical Equivalent”. The patient may then view a comparison of their with and without cylinder correction. This feature is also useful for contact lens patients considering a toric lens versus a spherical equivalent to correct low astigmatism.



This allows the patient to visualize the potential post-surgical differences between a standard and Toric IOL

Rotary Prism Measuring System

With Topcon's exclusive Rotary Prism Technology, the KR-800S also provides unmatched accuracy and reliability. The innovative optical design incorporated into the KR-800S allows for accurate and reliable measurements with a pupil as small as ϕ 2mm.

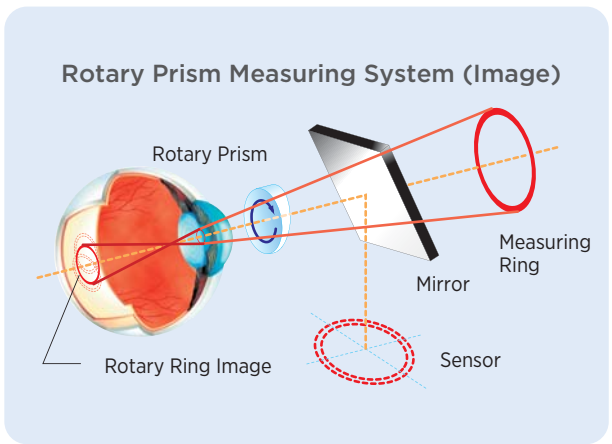

Topcon's Cataract Workstation

Cataract surgery quality control

Visual acuity (VA) is the most common clinical measure following cataract surgery. It is how we describe and measure the success of surgery. Measurement of VA must be standardized and systematic. Topcon's KR-800S Auto Kerato-refractometer with subjective VA check will do exactly that. With the KR-800S the VA can be subjectively tested pre- and post-operative cataract surgery. With the unique features of the KR-800S, such as “Glare” test and “Contrast” test, you can even evaluate the progression of cataract and identify cataract that is causing impaired quality of vision without a significant reduction in high contrast VA.

VA Simulation Premium IOL

KR-800S offers a Spherical Equivalent mode which can simulate the benefit of a premium (toric) IOL.

Cataract workstation

The KR-800S completes the screening workflow of cataract surgery. All necessary cataract pre-op information can be obtained by combining the KR-800S and ALADDIN, while the KR-800S assists you postop in Visual Acuity evaluation and determining the success of the cataract surgery. ALADDIN and KR-800S - the perfect combination for your cataract practice.

